



## Working with the DICOM and NIfTI Data Standards in R

Brandon Whitcher  
Mango Solutions

Volker J. Schmid  
Ludwig-Maximilians-  
Universität München

Andrew Thornton  
Cardiff University

---

### Abstract

Two packages, **oro.dicom** and **oro.nifti**, are provided for the interaction with and manipulation of medical imaging data that conform to the DICOM standard or ANALYZE/NIfTI formats. DICOM data, from a single file or directory tree, may be uploaded into R using basic data structures: a data frame for the header information and a matrix for the image data. A list structure is used to organize multiple DICOM files. The S4 class framework is used to develop basic ANALYZE and NIfTI classes, where NIfTI extensions may be used to extend the fixed-byte NIfTI header. One example of this, that has been implemented, is an XML-based “audit trail” tracking the history of operations applied to a data set. The conversion from DICOM to ANALYZE/NIfTI is straightforward using the capabilities of both packages. The S4 classes have been developed to provide a user-friendly interface to the ANALYZE/NIfTI data formats; allowing easy data input, data output, image processing and visualization.

*Keywords:* export, imaging, import, medical, visualization.

---

## 1. Introduction

Medical imaging is well established in both the clinical and research areas with numerous equipment manufacturers supplying a wide variety of modalities. The DICOM (Digital Imaging and Communications in Medicine; <http://medical.nema.org/>) standard was developed from earlier standards and released in 1993. It is the data format for clinical imaging equipment and a variety of other devices whose complete specification is beyond the scope of this paper. All major manufacturers of medical imaging equipment (e.g., GE, Siemens, Philips) have so-called DICOM conformance statements that explicitly state how their hardware implements DICOM. The DICOM standard provides interoperability across hardware, but was not designed to facilitate efficient data manipulation and image processing. Hence, additional

<b>oro.dicom</b>	
<code>create3D, create4D</code>	Create multi-dimensional arrays from DICOM header/image lists.
<code>dicom2analyze, dicom2nifti</code>	Convert DICOM objects to ANALYZE or NIfTI objects.
<code>dicomInfo, dicomSeparate dicomTable, writeHeader</code>	Read single or multiple DICOM files into R. Construct data frame from DICOM header list and write to a CSV file.
<code>extractHeader, header2matrix, matchHeader</code>	Extract information from DICOM headers.
<code>str2date, str2time</code>	Convert DICOM date or time entry into an R object.
<b>oro.nifti</b>	
<code>afni, anlz, nifti</code>	Class constructors for AFNI, ANALYZE and NIfTI objects.
<code>as(&lt;obj&gt;, "nifti")</code>	Coerce object into class <code>nifti</code> .
<code>audit.trail, aux.file, descrip</code>	Extract or replace slots in specific header fields.
<code>fmri2oro, oro2fmri</code>	Convert between <code>fmridata</code> ( <b>fmri</b> ) and <code>nifti</code> objects.
<code>hotmetal, tim.colors</code>	Useful color tables for visualization.
<code>image, orthographic, overlay</code>	Two-dimensional visualization methods.
<code>is.afni, is.anlz, is.nifti</code>	Logical checks.
<code>readAFNI, readANALYZE, readNIfTI</code>	Data input.
<code>writeAFNI, writeANALYZE, writeNIfTI</code>	Data output.

Table 1: List of functions available in **oro.dicom** and **oro.nifti**. Functionality around the AFNI data format was recently added to the **oro.nifti** package. Please visit <http://afni.nimh.nih.gov/afni/> for more information about the AFNI data format.

data formats have been developed over the years to accommodate data analysis and image processing.

The ANALYZE format was developed at the Mayo Clinic (in the 1990s) to store multidimensional biomedical images. It is fundamentally different from the DICOM standard since it groups all images from a single acquisition (typically three- or four-dimensional) into a pair of binary files, one containing header information and one containing the image information. The DICOM standard groups the header and image information, typically a single two-dimensional image, into a single file. Hence, a single acquisition will contain multiple DICOM files but only a pair of ANALYZE files.

The NIfTI format was developed in the early 2000s by the DFWG (Data Format Working Group) in an effort to improve upon the ANALYZE format. The resulting NIfTI-1 format adheres to the basic header/image combination from the ANALYZE format, but allows the pair of files to be combined into a single file and re-defines the header fields. In addition, NIfTI extensions allow one to store additional information (e.g., key acquisition parameters, experimental design) inside a NIfTI file.

The material presented here provides users with a method of interacting with DICOM, ANALYZE and NIfTI files in R (R Development Core Team 2010). Real-world data sets, that are

publicly available, are used to illustrate the basic functionality of the two packages: **oro.dicom** and **oro.nifti**. It should be noted that both packages focus on functions for data input/output and visualization. S4 classes **nifti** and **anlz** are provided for further statistical analysis in R without losing contextual information from the original ANALYZE or NIfTI files. Images in the metadata-rich DICOM format may be converted to NIfTI semi-automatically using as much information from the DICOM files as possible. Basic visualization functions, similar to those commonly used in the medical imaging community, are provided for **nifti** and **anlz** objects. Additionally, the **oro.nifti** package allows one to track every operation on a **nifti** object in an XML-based audit trail.

The **oro.dicom** and **oro.nifti** packages should appeal not only to R package developers, but also to scientists and researchers who want to interrogate medical imaging data using the statistical capabilities of R without writing and validating their own basic data input/output functionality. Table 1 lists the key functions for both packages and groups them according to common functionality. An example of using statistical methodology in R for the analysis of functional magnetic resonance imaging (fMRI) data is given in Section 3.7. Packages already available on the Comprehensive R Archive Network (CRAN, <http://CRAN.R-project.org/>) that utilize **oro.dicom** and **oro.nifti** include **cudaBayesreg** (Ferreira da Silva 2010a; Ferreira da Silva 2011), **dcmriS4** (Whitcher and Schmid 2011a,b), **dpmixsim** (Ferreira da Silva 2010b), and **RNiftyReg** (Clayden 2011).

## 2. oro.dicom: DICOM data input/output in R

The DICOM “standard” for data acquired using a clinical imaging device is very broad and complex. Roughly speaking each DICOM-compliant file is a collection of fields organized into two two-byte sequences (group,element) that are represented as hexadecimal numbers and form a tag. The (group,element) combination establishes what type of information is forthcoming in the file. There is no fixed number of bytes for a DICOM header. The final (group,element) tag should be the “pixel data” tag (7FE0,0010), such that all subsequent information is related to the image(s).

All attributes in the DICOM standard require different data types for correct representation. These are known as value representations (VRs) in DICOM, which may be encoded explicitly or implicitly. There are 27 explicit VRs defined in the DICOM standard. Detailed explanations of these data types are provided in the Section 6.2 (part 5) of the DICOM standard (<http://medical.nema.org/>). Internal functions have been written to manipulate each of the value representations and are beyond the scope of this article. The functions **str2date** and **str2time** are useful for converting from the DICOM **Datetime** and **Time** value representations to R date and time objects, respectively.

### 2.1. The DICOM header

Accessing the information stored in a single DICOM file is provided using the **dicomInfo** function. The basic structure of a DICOM file is summarized in Figure 1, for both explicit and implicit value representations. The first two bytes represent the **group** tag and the second two bytes represent the **element** tag, regardless of the type of VR. The third set of two bytes contains the characters of the VR on which a decision about being implicit or explicit is made. Explicit VRs of type (OB, OF, OW, SQ, UT, UN) skip bytes six and seven (counting from

---

Data element with explicit VR of OB, OF, OW, SQ, UT or UN:

```
+-----+
| 0 | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 |
+-----+
|<Group-->|<Element>|<VR----->|<0x0000->|<Length----->|<Value->
```

Data element with explicit VR other than as shown above:

```
+-----+
| 0 | 1 | 2 | 3 | 4 | 5 | 6 | 7 |
+-----+
|<Group-->|<Element>|<VR----->|<Length->|<Value->
```

Data element with implicit VR:

```
+-----+
| 0 | 1 | 2 | 3 | 4 | 5 | 6 | 7 |
+-----+
|<Group-->|<Element>|<Length----->|<Value->
```

---

Figure 1: Byte ordering for a single (group,element) tag in the DICOM standard. Explicit VRs store the VR as text characters in two bytes. More information is provided in Section 7, Part 3.5-2009 of the DICOM standard (<http://medical.nema.org/>).

zero), convert the next four bytes into an integer **length** and read **length** number of objects from the DICOM file. All other explicit VRs follow a slightly different path where bytes six and seven (counting from zero) provide an integer **length** and all remaining bytes are read in as the **value**. If the character string in bytes four and five do not correspond to a known VR (Figure 1), then the (group,element) tag is declared to be implicit, the **length** is taken from bytes four through seven and all remaining bytes contribute to the **value**.

The basic structure of the resulting object is a list with two elements: the DICOM header (**hdr**) and the DICOM image (**img**). The header information is organized in a data frame with six columns and an unknown number of rows depending on the input parameters.

```
R> fname <- system.file(file.path("dcm", "Abdo.dcm"), package = "oro.dicom")
R> abdo <- dicomInfo(fname)
R> names(abdo)
```

```
[1] "hdr" "img"
```

```
R> head(abdo$hdr)
```

	group	element		name	code	length
1	0002	0000		GroupLength	UL	4

```

2 0002 0001 FileMetaInformationVersion OB 2
3 0002 0002 MediaStorageSOPClassUID UI 26
4 0002 0003 MediaStorageSOPInstanceUID UI 38
5 0002 0010 TransferSyntaxUID UI 20
6 0002 0012 ImplementationClassUID UI 16
      value sequence
1      166
2      skipped
3      1.2.840.10008.5.1.4.1.1.4
4 1.3.46.670589.11.0.4.1996082307380007
5      1.2.840.10008.1.2.1
6      1.3.46.670589.17

```

```
R> tail(abdo$hdr)
```

```

      group element      name code length value sequence
79 0028 0101 BitsStored US 2 12
80 0028 0102 HighBit US 2 11
81 0028 0103 PixelRepresentation US 2 0
82 0028 1050 WindowCenter DS 4 530
83 0028 1051 WindowWidth DS 4 1052
84 7FE0 0010 PixelData OW 131072

```

The ordering of the rows is identical to the ordering in the original DICOM file. Hence, the first five tags in the DICOM header of `Abdo.dcm` are: `GroupLength`, `FileMetaInformationVersion`, `MediaStorageSOPClassUID`, `MediaStorageSOPInstanceUID` and `TransferSyntaxUID`. The last five tags in the DICOM header are also shown, with the very last tag indicating the start of the image data for that file and the number of bytes (131072) involved. When additional tags in the DICOM header information are queried (via `extractHeader`)

```
R> extractHeader(abdo$hdr, "BitsAllocated")
```

```
[1] 16
```

```
R> extractHeader(abdo$hdr, "Rows")
```

```
[1] 256
```

```
R> extractHeader(abdo$hdr, "Columns")
```

```
[1] 256
```

it is clear that the data are consistent with the header information in terms of the number of bytes ( $256 \times 256 \times (16/8) = 131072$ ).

The first five columns are taken directly from the DICOM header information (`group`, `element`, `code`, `length` and `value`) or inferred from that information (`name`). Note, the (`group`,`element`)

values are stored as character strings even though they are hexadecimal numbers. All aspects of the data frame may be interrogated in R in order to extract relevant information from the DICOM header; e.g., "BitsAllocated" as above. The `sequence` column is used to keep track of tags that are embedded in a fixed-length `SequenceItems` tag or between a `SequenceItem-SequenceDelimitationItem` pair.

When multiple DICOM files are located in a single directory, or spread across multiple directories, one may use the function `dicomSeparate` (applied here to the directory `hk-40`).

```
R> fname <- system.file("hk-40", package = "oro.dicom")
R> hk40 <- dicomSeparate(fname, verbose = TRUE, counter = 10)
```

```
40 files to be processed!
10 files processed...
20 files processed...
30 files processed...
40 files processed...
```

```
R> unlist(lapply(hk40, length))
```

```
hdr img
40 40
```

The object associated with `dicomSeparate` is now a nested set of lists, where the `hdr` element is a list of data frames and the `img` element is a list of matrices. These two lists are associated in a pairwise sense; i.e., `hdr[[1]]` is the header information for the image `img[[1]]`. Default parameters `recursive = TRUE` and `pixelData = TRUE` (which is actually an input parameter for `dicomInfo`) allow the user to search down all possible sub-directories and upload the image in addition to the header information, respectively. Also, by default all files are treated as DICOM files unless the `exclude` parameter is set to the unwanted file extension; e.g., `exclude = "xml"`.

The list of DICOM header information across multiple files may be converted to a single data frame using `dicomTable`, and written to disc for further analysis; e.g., using `write.csv`.

```
R> hk40.info <- dicomTable(hk40$hdr)
R> write.csv(hk40.info, file = "hk40_header.csv")
R> sliceloc.col <- which(hk40$hdr[[1]]$name == "SliceLocation")
R> sliceLocation <- as.numeric(hk40.info[, sliceloc.col])
R> head(sliceLocation)
```

```
[1] 160.9315 157.8315 154.7315 151.6315 148.5315 145.4315
```

```
R> head(diff(sliceLocation))
```

```
[1] -3.1 -3.1 -3.1 -3.1 -3.1 -3.1
```

```
R> unique(extractHeader(hk40$hdr, "SliceThickness"))
```

```
[1] 3.125
```

The tag `SliceLocation` is extracted from the DICOM header information (at the first element in the list) and processed using the `diff` function, and should agree with the `SliceThickness` tag. Single DICOM fields may also be extracted from the list of DICOM header information that contain attributes that are crucial for further image processing; e.g., extracting relevant MR sequences or acquisition timings.

```
R> head(extractHeader(hk40$hdr, "SliceLocation"))

[1] 160.9315 157.8315 154.7315 151.6315 148.5315 145.4315

R> modality <- extractHeader(hk40$hdr, "Modality", numeric = FALSE)
R> head(matchHeader(modality, "mr"))

[1] TRUE TRUE TRUE TRUE TRUE TRUE

R> (seriesTime <- extractHeader(hk40$hdr, "SeriesTime", numeric = FALSE))

[1] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[5] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[9] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[13] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[17] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[21] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[25] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[29] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[33] "113751.966000" "113751.966000" "113751.966000" "113751.966000"
[37] "113751.966000" "113751.966000" "113751.966000" "113751.966000"

R> str2time(seriesTime)

$txt
[1] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[5] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[9] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[13] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[17] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[21] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[25] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[29] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[33] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"
[37] "11:37:51.96600" "11:37:51.96600" "11:37:51.96600" "11:37:51.96600"

$time
[1] 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97
[8] 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97
[15] 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97
[22] 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97
[29] 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97 41871.97
[36] 41871.97 41871.97 41871.97 41871.97 41871.97
```



Figure 2: Coronal slice of the abdomen viewed in *neurological* convention (left is right and right is left).

## 2.2. The DICOM image

Most DICOM files involve a single slice from an acquisition – the image. A notable exception is the Siemens MOSAIC format (addressed in Section 2.2.1). The **oro.dicom** package assumes the image is stored as a flat file of two-byte integers without compression. A variety of additional image formats are possible within the DICOM standard; e.g., RGB-colored, JPEG, JPEG Lossless, JPEG 2000 and run-length encoding (RLE). None of these formats are currently available in **oro.dicom**. Going back to the `Abdo.dcm` example, the image is accessed via

```
R> image(t(abdo$img), col = grey(0:64/64), axes = FALSE, xlab = "",
+       ylab = "")
```

where the transpose operation is necessary for proper visualization of the image. Figure 2 displays a coronal slice through the abdomen from an MRI acquisition. All information from the original data acquisition should accompany the image through the DICOM header, and this information is utilized as much as possible by **oro.dicom** to simplify the manipulation of DICOM data. As previously shown, this information is easily available to the user by matching DICOM header fields with valid strings. Note, the function `extractHeader` assumes the output should be coerced via `as.numeric` but this may be disabled setting the input parameter `numeric = FALSE`.

```
R> extractHeader(abdo$hdr, "Manufacturer", numeric = FALSE)
```

```
[1] "Philips"
```



```
R> extractHeader(abdo$hdr, "RepetitionTime")
```

```
[1] 2000
```

```
R> extractHeader(abdo$hdr, "EchoTime")
```

```
[1] 100
```

The basic DICOM file structure does not encourage the analysis of multi-dimensional imaging data (e.g., 3D or 4D) commonly acquired on clinical scanners. Hence, the **oro.dicom** package has been developed to access DICOM files and facilitate their conversion to the NIfTI or ANALYZE formats in R. The conversion process requires the **oro.nifti** package and will be outlined in Section 4.

### *Siemens MOSAIC format*

Siemens multi-slice EPI (echo planar imaging) data may be collected as a “mosaic” image; i.e., all slices acquired in a single TR (repetition time) frame of a dynamic run are stored in a single DICOM file. The images are stored in an  $M \times N$  array of images. The function `create3D` will try to guess the number of images embedded within the single DICOM file using the `AcquisitionMatrix` field. If this doesn’t work, one may enter the  $(M, N)$  doublet explicitly.

```
R> fname <- system.file(file.path("dcm", "MR-sonata-3D-as-Tile.dcm"),
+   package = "oro.dicom")
R> dcm <- dicomInfo(fname)
R> dim(dcm$img)
```

```
[1] 384 384
```

```
R> dcmImage <- create3D(dcm, mosaic = TRUE)
R> dim(dcmImage)
```

```
[1] 64 64 36
```

Figure 3a is taken from the raw DICOM file, in mosaic format, and displayed with the default margins in R. Figure 3b is displayed after re-organizing the original DICOM file into a three-dimensional array (it was also converted to the NIfTI format for ease of visualization using the overloaded `image` function in **oro.nifti**).

## 3. **oro.nifti**: NIfTI-1 data input/output in R

Although the industry standard for medical imaging data is DICOM, another format has come to be heavily used in the image analysis community. The ANALYZE format was originally developed in conjunction with an image processing system (of the same name) at the Mayo Foundation. A common version of the format, although not the most recent, is called

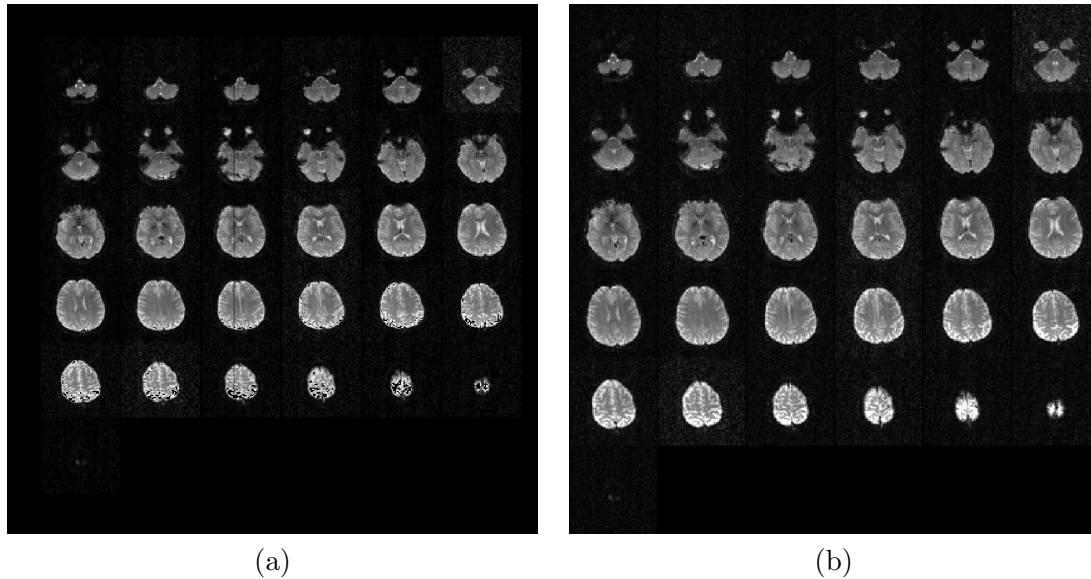


Figure 3: (a) Single MOSAIC image as read in from `dicomInfo`. (b) Lightbox display of three-dimensional array of images after processing via `create3D`.

ANALYZE 7.5. A copy of the file `ANALYZE75.pdf` has been included in `oro.nifti` (accessed via `system.file("doc/ANALYZE75.pdf", package = "oro.dicom")`) since it does not appear to be available from <http://www.mayo.edu/> any longer. An ANALYZE 7.5 format image is comprised of two files, the `.hdr` and `.img` files, that contain information about the acquisition and the acquisition itself, respectively. A more recent adaption of this format is known as NIfTI-1 and is a product of the Data Format Working Group (DFWG) from the Neuroimaging Informatics Technology Initiative (NIfTI; <http://nifti.nimh.nih.gov/>). The NIfTI-1 data format is almost identical to the ANALYZE format, but offers a few improvements:

- Merging of the header and image information into one file (`.nii`).
- Re-organization of the 348-byte fixed header into more relevant categories .
- Possibility of extending the header information.

There are several R packages that also offer input/output functionality for the NIfTI and ANALYZE data formats in addition to image analysis capabilities for specific MRI acquisition sequences; e.g., **AnalyzeFMRI** (Marchini and Lafaye de Micheaux 2009; Bordier *et al.* 2011), **fmri** (Tabelow and Polzehl 2011) and **tractar.base** (Clayden 2010; Clayden *et al.* 2011). The **Rniftilib** package provides access to NIfTI data via the **nifticlib** library (Granert 2010).

### 3.1. The NIfTI header

The NIfTI header inherits its structure (348 bytes in length) from the ANALYZE data format. The last four bytes in the NIfTI header correspond to the “magic” field and denote whether or not the header and image are contained in a single file (`magic = "n+1\0"`) or two separate files (`magic = "ni1\0"`), the latter being identical to the structure of the ANALYZE data format. The NIfTI data format added an additional four bytes to allow for “extensions” to the header. By default these four bytes are set to zero.

The first example of reading in, and displaying, medical imaging data in NIfTI format `avg152T1_LR_nifti.nii.gz` was obtained from the NIfTI website (<http://nifti.nimh.nih.gov/nifti-1/>). Successful execution of the commands

```
R> fname <- system.file(file.path("nifti", "mniLR.nii.gz"),
+   package = "oro.nifti")
R> (mniLR <- readNIfTI(fname))
```

NIfTI-1 format

```
Type           : niftiAuditTrail
Data Type      : 2 (UINT8)
Bits per Pixel : 8
Slice Code     : 0 (Unknown)
Intent Code    : 0 (None)
Qform Code     : 0 (Unknown)
Sform Code     : 4 (MNI_152)
Dimension      : 91 x 109 x 91
Pixel Dimension : 2 x 2 x 2
Voxel Units    : mm
Time Units     : sec
```

```
R> aux.file(mniLR)
```

```
[1] "none"
```

```
R> descrip(mniLR)
```

```
[1] "FSL3.2beta"
```

produces an S4 "nifti" object (or "niftiAuditTrail" if the audit trail option is set). Two accessor functions are also provided: `aux.file` and `descrip`. The former is used to access the original name of the file (if it has been provided) and the latter is the name of a valid NIfTI header field used to hold a "description" (up to 80 characters in length).

### 3.2. The NIfTI image

Image information begins at the byte position determined by the `voxoffset` slot. In a single NIfTI file (`magic = "n+1\0"`), this is by default after the first 352 bytes. Header extensions extend the size of the header and come before the image information leading to a consequent increase of `voxoffset` for single NIfTI files. The split NIfTI (`magic = "ni1\0"`) and ANALYZE formats contain pairs of files, where the header and image information are separated, and do not have this problem. In this case `voxoffset` is set to 0.

The `image` function has been overloaded so that it behaves differently when dealing with medical image objects (`nifti` and `anlz`). The command

```
R> image(mniLR)
```

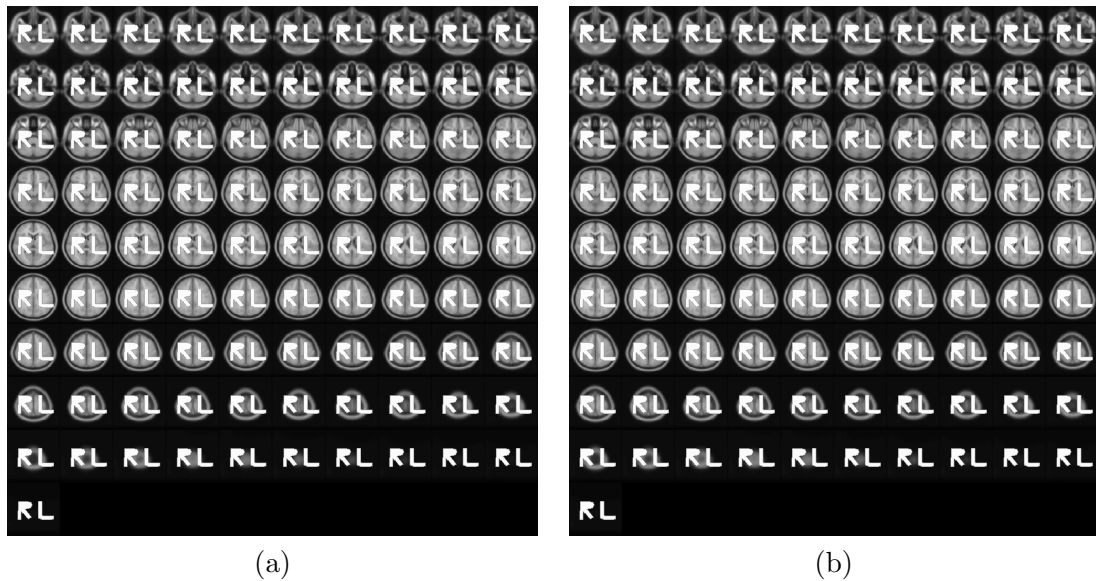


Figure 4: (a) Axial slices of MNI volume `mniLR_nifti` stored in the *neurological* convention (right-is-right), but displayed in the *radiological* convention (right-is-left). (b) Axial slices of MNI volume `mniRL_nifti` stored and displayed in the *radiological* convention.

produces a three-dimensional array of the MNI brain, with the default NIfTI axes, and is displayed on a 10×10 grid of images (Figure 4a). The `image` function for medical image S4 objects is an attempt to balance minimal user input with enough flexibility to customize the display when necessary. For example, single slices may be viewed by using the option `plot.type = "single"` in conjunction with the option `z =` to specify the slice.

The second example of reading in and displaying medical imaging data in the NIfTI format `avg152T1_RL_nifti.nii.gz` was also obtained from the NIfTI website (<http://nifti.nimh.nih.gov/nifti-1/>). Successful execution of the commands

```
R> fname <- system.file(file.path("nifti", "mniRL.nii.gz"),
+   package = "oro.nifti")
R> (mniRL <- readNIfTI(fname))
```

NIfTI-1 format

```
Type           : niftiAuditTrail
Data Type       : 2 (UINT8)
Bits per Pixel  : 8
Slice Code      : 0 (Unknown)
Intent Code     : 0 (None)
Qform Code      : 0 (Unknown)
Sform Code      : 4 (MNI_152)
Dimension       : 91 x 109 x 91
Pixel Dimension : 2 x 2 x 2
Voxel Units     : mm
Time Units      : sec
```

```
R> image(mniRL)
```

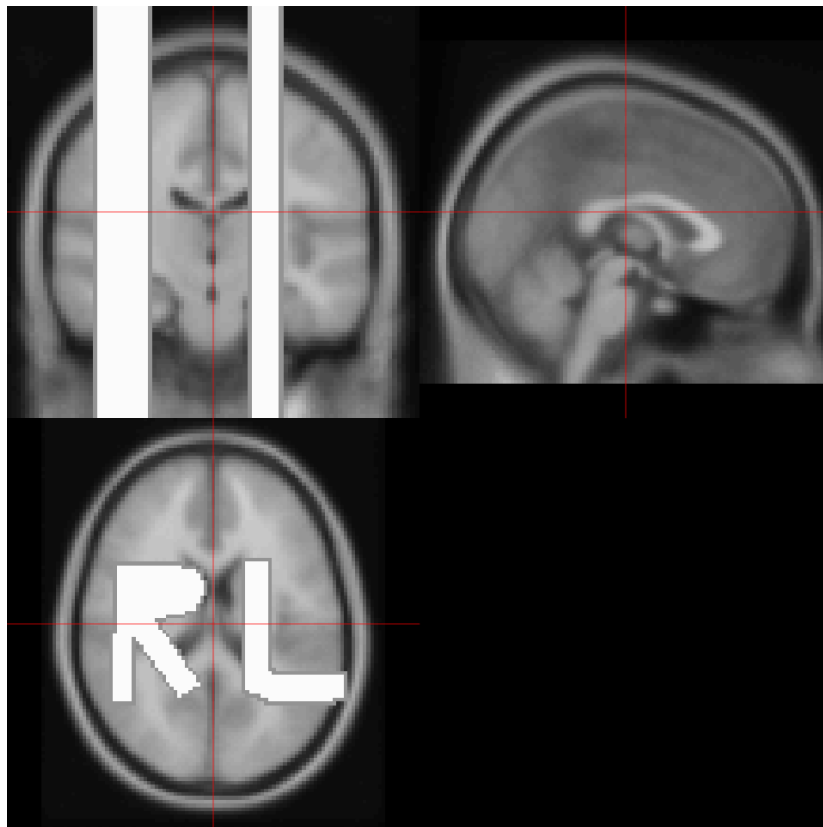


Figure 5: Orthographic display of the MNI volume `mniRL_nifti`. By default the mid-axial, mid-sagittal and mid-coronal planes are chosen.

produces a three-dimensional array of the MNI brain that is displayed in a  $10 \times 10$  grid of images (Figure 4b). The two sets of data in Figure 4 are stored in two different orientations, commonly referred to as the *radiological* and *neurological* conventions. The neurological convention is where “right is right” and one is essentially looking through the subject. The radiological convention is where “right is left” and one is looking at the subject. An additional graphical display function has been added for `nifti` and `anlz` objects that allows a so-called orthographic visualization of the data.

```
R> orthographic(mniRL)
```

As seen in Figure 5 the mid-axial, mid-sagittal and mid-coronal planes are displayed by default. The slices used may be set using `xyz = c(I,J,K)`, where  $(I, J, K)$  are appropriate indices, and the crosshairs will provide a spatial reference in each plane relative to the other two.

### 3.3. A note on axes and orientation

The NIfTI format contains an implicit generalized spatial transformation from the data co-ordinate system  $(i, j, k)$  into a real-space “right-handed” co-ordinate system. In this real-space system, the  $(x, y, z)$  axes are *usually* set such that  $x$  increases from left to right,  $y$  increases from posterior to anterior and  $z$  increases from inferior to superior.

At this point in time the **oro.nifti** package cannot apply an arbitrary transform to the imaging data into  $(x, y, z)$  space – such a transform may require non-integral indices and interpolation steps. The package does accommodate straightforward transformations of imaging data; e.g., setting the  $i$ -axis to increase from right to left (the neurological convention). Future versions of **oro.nifti** will attempt to address more complicated spatial transformations and provide functionality to display the  $(x, y, z)$  axes on orthographic plots.

### 3.4. NIfTI and ANALYZE data in S4

A major improvement in the **oro.nifti** package is the fact that standard medical imaging formats are stored in unique classes under the S4 system (Chambers 2008). Essentially, NIfTI and ANALYZE data are stored as multi-dimensional arrays with extra slots created that capture the format-specific header information; e.g., for a **nifti** object

```
R> slotNames(mniRL)
```

[1] ".Data"	"trail"	"extensions"	"sizeof_hdr"
[5] "data_type"	"db_name"	"extents"	"session_error"
[9] "regular"	"dim_info"	"dim_"	"intent_p1"
[13] "intent_p2"	"intent_p3"	"intent_code"	"datatype"
[17] "bitpix"	"slice_start"	"pixdim"	"vox_offset"
[21] "scl_slope"	"scl_inter"	"slice_end"	"slice_code"
[25] "xyzt_units"	"cal_max"	"cal_min"	"slice_duration"
[29] "toffset"	"glmax"	"glmin"	"descrip"
[33] "aux_file"	"qform_code"	"sform_code"	"quatern_b"
[37] "quatern_c"	"quatern_d"	"qoffset_x"	"qoffset_y"
[41] "qoffset_z"	"srow_x"	"srow_y"	"srow_z"
[45] "intent_name"	"magic"	"extender"	"reoriented"

```
R> c(mniRL@cal_min, mniRL@cal_max)
```

```
[1] 0 255
```

```
R> range(mniRL)
```

```
[1] 0 255
```

```
R> mniRL@datatype
```

```
[1] 2
```

```
R> convert.datatype(mniRL@datatype)
```

```
[1] "UINT8"
```

Note, an ANALYZE object has a slightly different set of slots. Slots 4–47 are taken verbatim from the definition of the NIfTI format and are read directly from a file. The slot **.Data** is the multidimensional array (since class **nifti** inherits from class **array**) and the slots **trail**, **extensions** and **reoriented** are used for internal bookkeeping. In the code above we have accessed the min/max values of the imaging data using the "cal\_min" and "cal\_max" slots

and matches a direct interrogation of the `.Data` slot using the `range` function. Looking at the `datatype` slot provides a numeric code that may be converted into a value that indicates the type of byte structure used (in this case an 8-bit or 1-byte unsigned integer).

As introduced in Section 3.1 there are currently only two accessor functions to slots in the NIfTI header (`aux.file` and `descrip`) – all other slots are either ignored or used inside of functions that operate on ANALYZE/NIfTI objects. The NIfTI class also has the ability to read and write extensions that conform to the NIfTI data format. Customized printing and validity-checking functions are available to the user and every attempt has been made to ensure that the information from the multi-dimensional array is in agreement with the header values.

The constructor function `nifti` produces valid NIfTI objects, including a consistent header, from an arbitrary array.

```
R> n <- 100
R> (random.image <- nifti(array(runif(n * n), c(n, n, 1))))
```

NIfTI-1 format

```
Type           : niftiAuditTrail
Data Type       : 2 (UINT8)
Bits per Pixel  : 8
Slice Code      : 0 (Unknown)
Intent Code     : 0 (None)
Qform Code      : 0 (Unknown)
Sform Code      : 0 (Unknown)
Dimension       : 100 x 100 x 1
Pixel Dimension : 1 x 1 x 1
Voxel Units     : Unknown
Time Units      : Unknown
```

```
R> random.image@dim_
```

```
[1]  3 100 100  1  1  1  1  1
```

```
R> dim(random.image)
```

```
[1] 100 100  1
```

The function `writeNifti` outputs valid NIfTI class files, which can be opened in other medical imaging software. Files can either be stored as standard `.nii` files or compressed with `gzip` (default).

```
R> writeNifti(random.image, "random")
R> list.files(pattern = "random")
```

```
[1] "random.nii.gz"
```



---

```
R> audit.trail(mniLR)

<audit-trail xmlns="http://www.dcemri.org/namespaces/audit-trail/1.0">
  <created>
    <workingDirectory>/home/guest/dicom_nifti</workingDirectory>
    <filename>/home/bwhitcher/R/x86_64-unknown-linux-gnu-library/2.13/
      oro.nifti/nifti/mniLR.nii.gz</filename>
    <call>readNIfTI(fname = fname)</call>
    <system>
      <r-version.version.string>R version 2.13.1 (2011-07-08)
      </r-version.version.string>
      <date>Sun Aug 21 09:29:36 2011 BST</date>
      <user>bwhitcher</user>
      <package-version.Version>0.2.7</package-version.Version>
    </system>
  </created>
</audit-trail>
```

---

Figure 6: XML-based audit trail obtained via `audit.trail(mniLR)`.

### 3.5. The audit trail

Following on from the S4 implementation of both the NIfTI and ANALYZE data formats, the ability to extend the NIfTI data format header is utilized in the **oro.nifti** package. First, extensions are properly handled when reading and writing NIfTI data. Second, users are allowed to add extensions to newly-created NIfTI objects by casting them as `niftiExtension` objects and adding `niftiExtensionSection` objects to the `extensions` slot. Third, by default all operations that are performed on a NIfTI object will generate what we call an *audit trail* that consists of an XML-based log (Temple Lang 2010). Each log entry contains information not only about the function applied to the NIfTI object, but also various system-level information; e.g., version of R, user name, date, time, etc. When writing NIfTI-class objects to disk, the XML-based NIfTI extension is converted into plain text and saved using `ecode = 6` to denote plain ASCII text only. The user may control the tracking of data manipulation via the audit trail using a global option. For example, please use the command

```
R> options(niftiAuditTrail = FALSE)
```

to turn off the “audit trail” option in **oro.nifti**. Figure 6 displays output from the accessor function `audit.trail(mniLR)`, the XML-based audit trail that is stored as a NIfTI header extension.

### 3.6. Interactive visualization

Basic visualization of `nifti` and `anlz` class images can be achieved with any visualization for arrays in R. For example, the **EBImage** package provides functions `display` and `animate` for visualization (Sklyar and Huber 2006; Sklyar *et al.* 2010). Please note that functions in **EBImage** expect grey-scale values in the range  $[0, 1]$ , hence the display of `nifti` data may be performed using



```
R> mniLR.range <- range(mniLR)
R> display((mniLR - min(mniLR))/diff(mniLR.range))
```

Interactive visualization of multi-dimensional arrays, stored in NIfTI or ANALYZE format, is however best performed outside of R at this point in time. Popular viewers, especially for neuroimaging data, include **FSLView** ([Analysis Group, FMRIB, Oxford 2011](#)), **MRICron** ([Rorden 2011](#)), **ITKSnap** ([Yushkevich et al. 2006](#)), and **VolView** ([Kitware, Inc. 2011](#)). The **mrirc** package provides basic interactive visualization of ANALYZE/NIfTI data using a Tcl/Tk interface ([Whitcher et al. 2011](#); [Feng and Tierney 2011](#)).

### 3.7. An example using functional MRI data

This is an example of reading in, and displaying, a four-dimensional medical imaging data set in NIfTI format `filtered_func_data` obtained from the **FSL** evaluation and example data suite ([Analysis Group, FMRIB, Oxford 2008](#)). Successful execution of the commands

```
R> (ffd <- readNIfTI("filtered_func_data"))
```

NIfTI-1 format

```
Type           : niftiAuditTrail
Data Type       : 16 (FLOAT32)
Bits per Pixel  : 32
Slice Code      : 0 (Unknown)
Intent Code     : 0 (None)
Qform Code      : 0 (Unknown)
Sform Code      : 0 (Unknown)
Dimension       : 64 x 64 x 21 x 180
Pixel Dimension : 4 x 4 x 6 x 3
Voxel Units     : mm
Time Units      : sec
```


```
R> image(ffd, zlim = range(ffd) * 0.85)
```

produces a four-dimensional (4D) array of imaging data that may be displayed in a 5×5 grid of images (Figure 7a). The first three dimensions are spatial locations of the voxel (volume element) and the fourth dimension is time for this functional MRI (fMRI) acquisition. As seen from the summary of object, there are 21 axial slices of fairly coarse resolution (4×4×6 mm) and reasonable temporal resolution (3 s). Figure 7b depicts the orthographic display of the `filtered_func_data` using the axial plane containing the left-and-right thalamus to approximately center the crosshair vertically.


```
R> orthographic(ffd, xyz = c(34, 29, 10), zlim = range(ffd) * 0.85)
```

#### *Statistical analysis*

The R programming environment provides a wide variety of statistical methodology for the quantitative analysis of medical imaging data. For example, fMRI data are typically analyzed

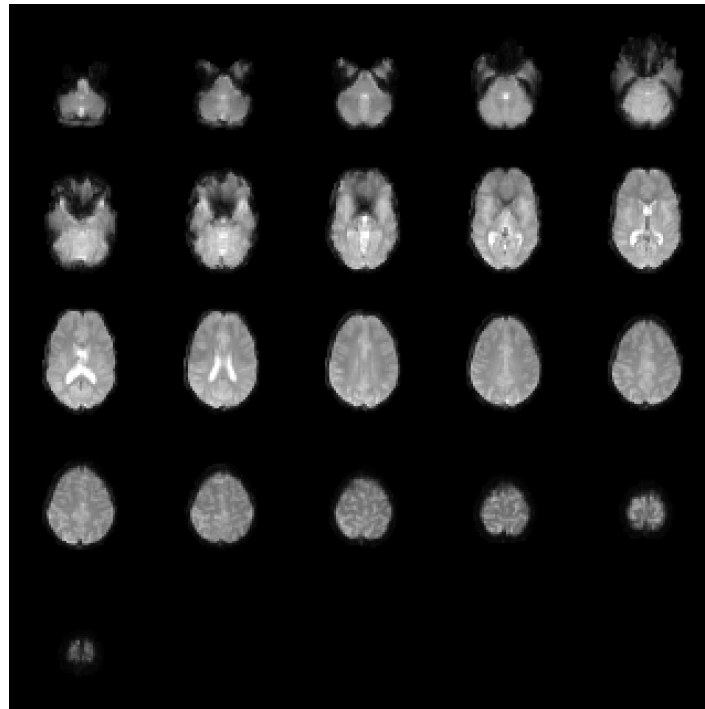

(a)

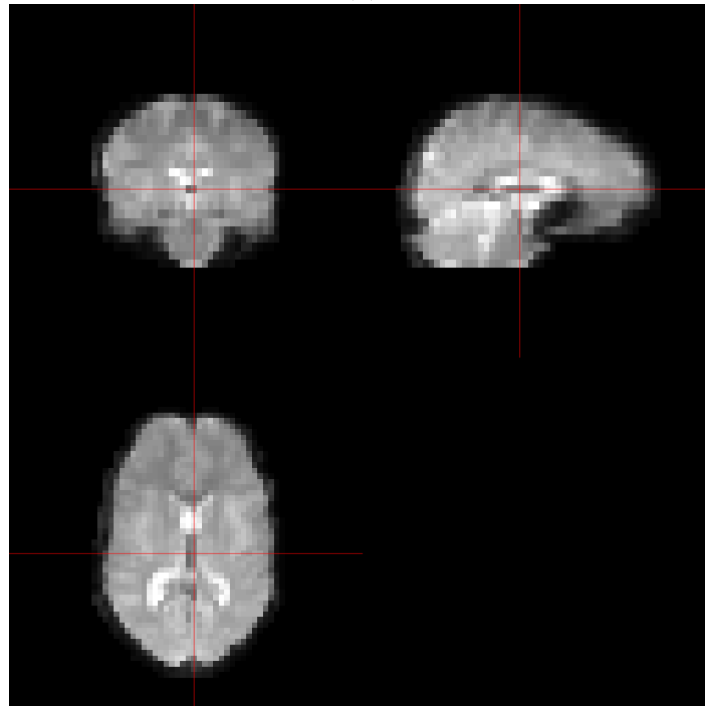

(b)

Figure 7: (a) Axial slices of the functional MRI data set `filtered_func_data` from the first acquisition. (b) Orthographic display of the first volume from the functional MRI data set `filtered_func_data`.

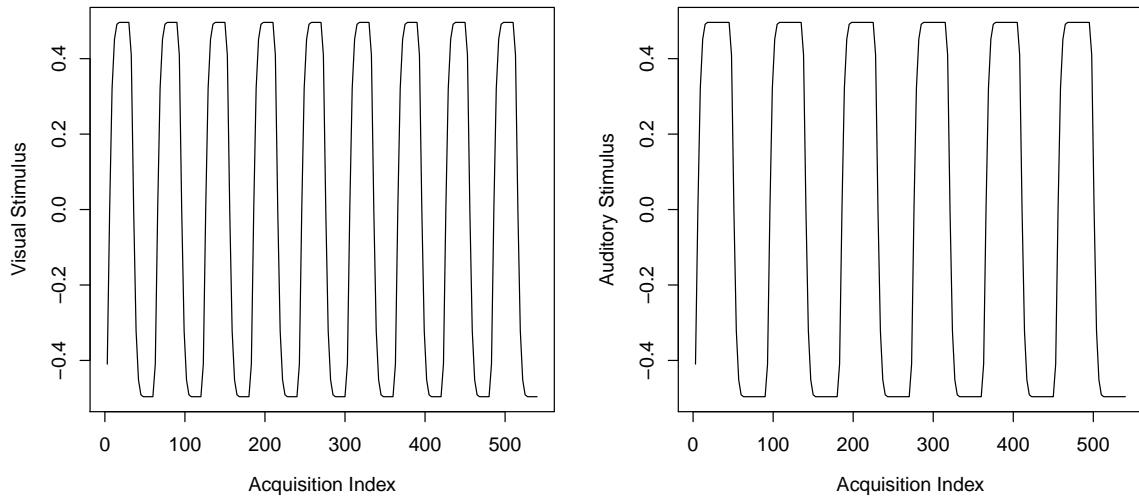


Figure 8: Visual (30 seconds on/off) and auditory (45 seconds on/off) stimuli, convolved with a parametric haemodynamic response function, used in the GLM-based fMRI analysis.

by applying a multiple linear regression model, commonly referred to in the literature as a general linear model (GLM), that utilizes the stimulus experiment to construct the design matrix. Estimation of the regression coefficients in the GLM produces a statistical image; e.g.,  $Z$  statistics for a voxel-wise hypothesis test on activation in fMRI experiments (Friston *et al.* 1994, 1995).

The 4D volume of imaging data in `filtered_func_data` was acquired in an experiment with a repetition time  $TR = 3$  s, using both visual and auditory stimuli. The visual stimulus was applied using an on/off pattern for a duration of 60 seconds and the auditory stimulus was applied using an on/off pattern for a duration of 90 seconds. A parametric haemodynamic response function (HRF), with mean  $\mu = 6$  and standard deviation  $\sigma = 3$ , is utilized here which is similar to the default values in **FSL** (Smith *et al.* 2004). We construct the experimental design and HRF in seconds, perform the convolution and then downsample by a factor of three in order to obtain columns of the design matrix that match the acquisition of the MRI data.

```
R> visual <- rep(c(-0.5, 0.5), each = 30, times = 9)
R> auditory <- rep(c(-0.5, 0.5), each = 45, times = 6)
R> hrf <- c(dgamma(1:15, 4, scale = 1.5))
R> hrf0 <- c(hrf, rep(0, length(visual) - length(hrf)))
R> visual.hrf <- convolve(hrf0, visual)
R> hrf0 <- c(hrf, rep(0, length(auditory) - length(hrf)))
R> auditory.hrf <- convolve(hrf0, auditory)
R> index <- seq(3, 540, by = 3)
R> visual.hrf <- visual.hrf[index]
R> auditory.hrf <- auditory.hrf[index]
```

Figure 8 depicts the visual and auditory stimuli, convolved with the HRF, in the order of

acquisition. The design matrix is then used in a voxel-wise GLM, where the `lsfit` function in R estimates the parameters in the linear regression. At each voxel  $t$  statistics and their associated  $p$  values are computed for the hypothesis test of no effect for each individual stimulus, along with an  $F$  statistic for the hypothesis test of no effect of any stimuli using the `ls.print` function.

```
R> voxel.lsfit <- function(x, thresh) {
+   if (max(x) < thresh) return(rep(NA, 5))
+   output <- lsfit(cbind(visual.hrf, auditory.hrf), x)
+   output.t <- ls.print(output, print.it = FALSE)$coef.table[[1]][2:3,3:4]
+   output.f <- ls.print(output, print.it = FALSE)$summary[3]
+   c(output.t, as.numeric(output.f))
+ }
R> ffd.glm <- apply(ffd, 1:3, voxel.lsfit, thresh = 0.1 * max(ffd))
```


Given the multidimensional array of output from the GLM fitting procedure, the  $t$  statistics are separated and converted into  $Z$  statistics to follow the convention used in **FSL**. For the purposes of this example we have not applied any multiple comparisons correction procedure and, instead, use a relatively large threshold of  $Z > 5$  for visualization.

```
R> dof <- ntim(ffd) - 1
R> Z.visual <- nifti(qnorm(pt(ffd.glm[1, , , ], dof, log.p = TRUE),
+   log.p = TRUE), datatype = 16)
R> Z.auditory <- nifti(qnorm(pt(ffd.glm[2, , , ], dof, log.p = TRUE),
+   log.p = TRUE), datatype = 16)
R> overlay(ffd, ifelse(Z.visual > 5, Z.visual, NA),
+   zlim.x = range(ffd) * 0.85, zlim.y = range(Z.visual, na.rm = TRUE))
R> overlay(ffd, ifelse(Z.auditory > 5, Z.auditory, NA),
+   zlim.x = range(ffd) * 0.85, zlim.y = range(Z.auditory, na.rm = TRUE))
```


Statistical images in neuroimaging are commonly displayed as an overlay on top of a reference image (one of the dynamic acquisitions) in order to provide anatomical context. The `overlay` command in **oro.nifti** allows one to display the statistical image of voxel-wise activations overlaid on one of the original EPI (echo planar imaging) volumes acquired in the fMRI experiment. The 3D array of  $Z$  statistics for the visual and auditory tasks are overlaid on the original data for “anatomical” reference in Figure 9. The  $Z$  statistics that exceed the threshold appear to match known neuroanatomy, where the visual cortex in the occipital lobe shows activation under the visual stimulus (Figure 9a) and the primary auditory cortex in the temporal lobe shows activation under the auditory stimulus (Figure 9b).

## 4. Converting DICOM to NIfTI

The **oro.dicom** and **oro.nifti** packages have been specifically designed to use as much information as possible from the metadata-rich DICOM format and apply that information in the construction of the NIfTI data volume. The function `dicom2nifti` converts a list of DICOM images into an **nifti** object, and likewise `dicom2analyze` converts such a list into an **anlz** object.

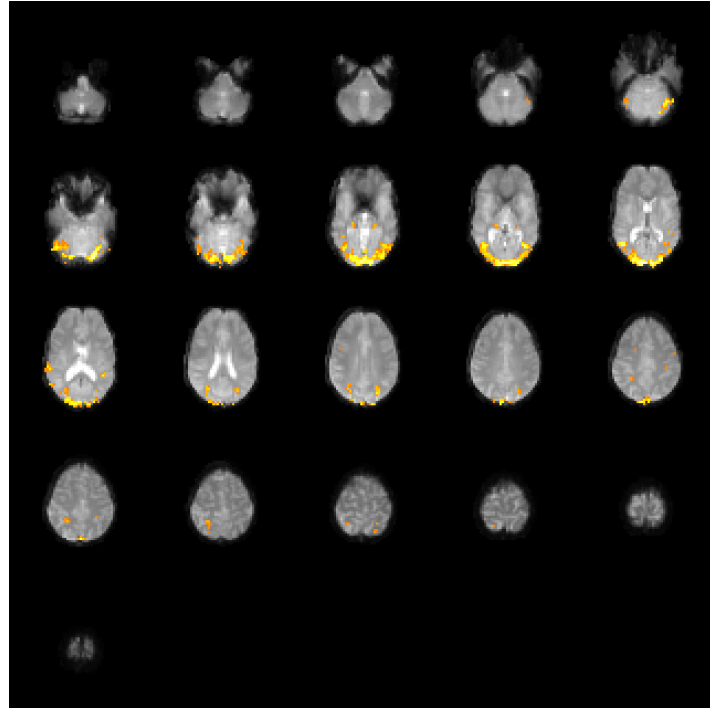

(a)

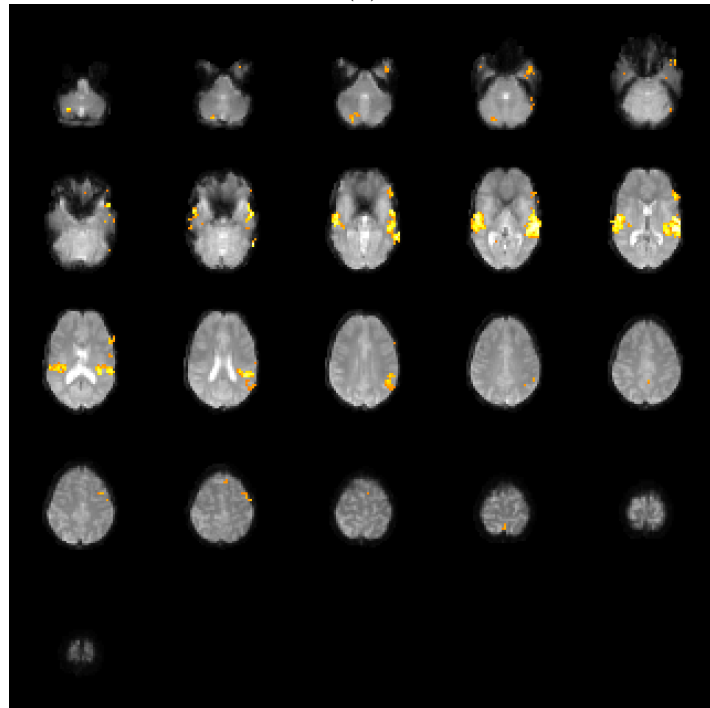

(b)

Figure 9: (a) Axial slices of the functional MRI data with the statistical image from the visual stimulus overlaid. (b) Axial slices of the functional MRI data with the statistical image from the auditory stimulus overlaid. Both sets of test statistics were thresholded at  $Z \geq 5$  for all voxel.

Historically, data conversion from DICOM to NIfTI (or ANALYZE) has been provided outside of R using one of several standalone software packages: **XMedCon** (Nolf 2003), **FreeSurfer** (Athinoula A. Martinos Center for Biomedical Imaging 2011), **MRIConvert** (Smith 2011). This is by no means an exhaustive list of software packages available for DICOM conversion. In addition there are several other R packages with the ability to process DICOM data: **fmri** (Tabelow and Polzehl 2011), **tractor.base** (Clayden 2010; Clayden *et al.* 2011, part of the tractor project <http://code.google.com/p/tractor>).

#### 4.1. An example using a single-series data set

Using the 40 images from the `hk40` object (previously defined in Section 2.1) it is straightforward to perform DICOM-to-NIfTI conversion using only default settings and plot the results in either lightbox or orthographic displays.

```
R> args(dicom2nifti)
```

```
function (dcm, datatype = 4, units = c("mm", "sec"), rescale = FALSE,
  reslice = TRUE, qform = TRUE, sform = TRUE, DIM = 3,
  descrip = "SeriesDescription", aux.file = NULL, ...)
NULL
```

```
R> (hk40n <- dicom2nifti(hk40))
```

NIfTI-1 format


```
Type           : niftiAuditTrail
Data Type       : 4 (INT16)
Bits per Pixel  : 16
Slice Code      : 0 (Unknown)
Intent Code     : 0 (None)
Qform Code      : 2 (Aligned_Anat)
Sform Code      : 2 (Aligned_Anat)
Dimension       : 256 x 256 x 40
Pixel Dimension : 1.56 x 1.56 x 3.12
Voxel Units     : mm
Time Units      : sec
```

```
R> image(hk40n)
```


```
R> orthographic(hk40n, col.crosshairs = "green")
```

By default `dicom2nifti` takes all image data from the DICOM list and creates a 3D image. Four-dimensional image volumes (three in space plus one in time) are also converted automatically by specifying `DIM = 4`, where slice positions are taken from the `ImagePositionPatient` DICOM header field. For example, using `DIM = 4` on the `hk40` DICOM data,

```
R> (hk40n <- dicom2nifti(hk40, DIM = 4))
```

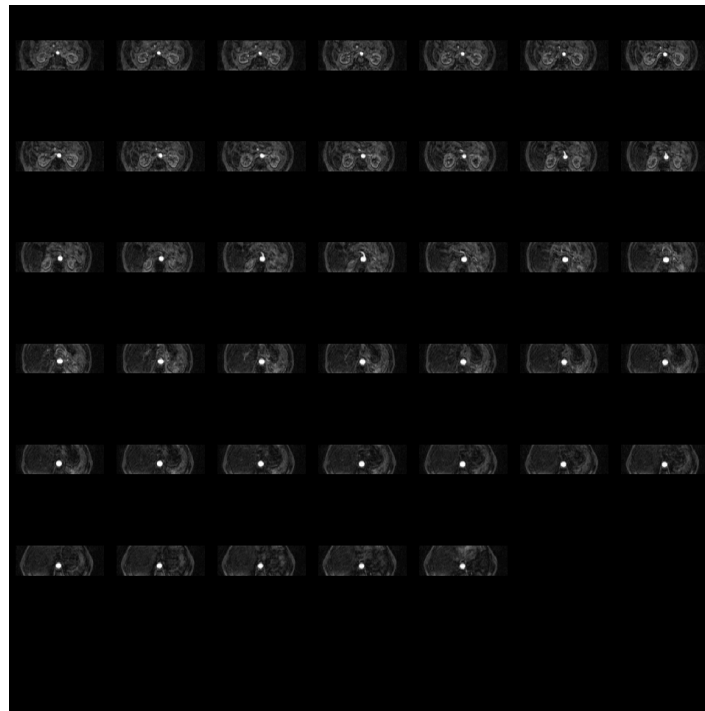

(a)

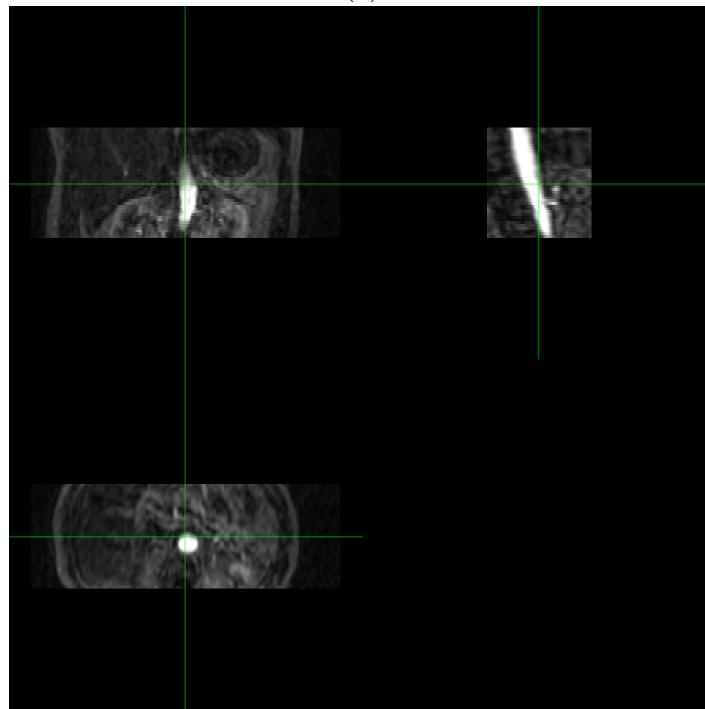

(b)

Figure 10: (a) Lightbox display of three-dimensional array of images. (b) Orthographic display of the same three-dimensional array (using the default settings for `orthographic`).

## NIfTI-1 format

```

Type           : niftiAuditTrail
Data Type      : 4 (INT16)
Bits per Pixel : 16
Slice Code     : 0 (Unknown)
Intent Code    : 0 (None)
Qform Code     : 2 (Aligned_Anat)
Sform Code     : 2 (Aligned_Anat)
Dimension      : 256 x 256 x 40
Pixel Dimension : 1.56 x 1.56 x 3.12
Voxel Units    : mm
Time Units     : sec

```

will also produce a three-dimensional volume of images, since the `ImagePositionPatient` field is unique for each single slice of the volume.

The functions `dicom2nifti` and `dicom2analyze` will fail when the dimensions of the individual images in the DICOM list do not match. However, they do not check for different series numbers or patient IDs so caution should be exercised when scripting automated work flows for DICOM-to-NIfTI conversion. In cases where a DICOM file includes images from more than one series, the corresponding slices have to be chosen before conversion, using `dicomTable`, `extractHeader`, and `matchHeader`.

## 4.2. An example using a multiple-volume data set

The National Biomedical Imaging Archive (NBIA; <http://cabig.nci.nih.gov/tools/NCIA>) is a searchable, national repository integrating *in vivo* cancer images with clinical and genomic data. The NBIA provides the scientific community with public access to DICOM images, image markup, annotations, and rich metadata. The multiple MRI sequences processed here were downloaded from the “RIDER Neuro MRI” collection at <http://wiki.nci.nih.gov/display/CIP/RIDER>. A small `for` loop has been written to operate on a subset of the DICOM directory structure, where the `SeriesInstanceUID` DICOM header field is assumed to be 100% accurate in series differentiation.

```

R> subject <- "1086100996"
R> DCM <- dicomSeparate(subject, verbose = TRUE, counter = 100)

564 files to be processed!
100 files processed...
200 files processed...
300 files processed...
400 files processed...
500 files processed...

R> seriesInstanceUID <- extractHeader(DCM$hdr, "SeriesInstanceUID",
+   FALSE)
R> for (uid in unique(seriesInstanceUID)) {
+   index <- which(unlist(lapply(DCM$hdr, function(x) uid %in% x$value)))

```



```

+   uid.dcm <- list(hdr = DCM$hdr[index], img = DCM$img[index])
+   patientsName <- extractHeader(uid.dcm$hdr, "PatientsName", FALSE)
+   studyDate <- extractHeader(uid.dcm$hdr, "StudyDate", FALSE)
+   seriesDescription <- extractHeader(uid.dcm$hdr, "SeriesDescription",
+   FALSE)
+   fname <- paste(gsub("[^0-9A-Za-z]", "", unique(c(patientsName,
+   studyDate, seriesDescription))), collapse = "_")
+   cat("##  ", fname, fill = TRUE)
+   if (gsub("[^0-9A-Za-z]", "", unique(seriesDescription)) == "axtensor") {
+     D <- 4
+     reslice <- FALSE
+   } else {
+     D <- 3
+     reslice <- TRUE
+   }
+   uid.nifti <- dicom2nifti(uid.dcm, DIM = D, reslice = reslice,
+   descrip = c("PatientID", "SeriesDescription"))
+   writeNIfTI(uid.nifti, fname)
+ }

##  281949_19040720_axtensor
##  281949_19040720_ax30flip
##  281949_19040720_ax15flip
##  281949_19040720_ax25flip
##  281949_19040720_ax20flip
##  281949_19040720_ax10flip
##  281949_19040720_ax5flip

```

Note, the diffusion tensor imaging (DTI) data **axtensor** is assumed to be four dimensional and all other series (the multiple flip-angle acquisitions) are assumed to be three dimensional. There is always a balance between what information should be pre-specified versus what can easily be extracted from the DICOM headers or images.

## 5. Conclusion

Medical image analysis depends on the efficient manipulation and conversion of DICOM data. The **oro.dicom** and **oro.nifti** packages have been developed to provide the user with a set of functions that mask as many of the background details as possible while still providing flexible and robust performance.

The future of medical image analysis in R will benefit from a unified view of the imaging data standards: DICOM, NIfTI and ANALYZE. The existence of a single package for handling imaging data formats would facilitate interoperability between the ever increasing number of R packages devoted to medical image analysis. We do not assume that the data structures in **oro.dicom** or **oro.nifti** are best-suited for this purpose and we welcome an open discussion around how best to provide this standardization to the end user.

## Acknowledgments

The authors would like to thank the National Biomedical Imaging Archive (NBIA), the National Cancer Institute (NCI), the National Institute of Health (NIH) and all institutions that have contributed medical imaging data to the public domain. The authors would also like to thank K. Tabelow for providing functionality around the AFNI data format. VS is supported by the German Research Council (DFG SCHM 2747/1-1).

## References

- Analysis Group, FMRI, Oxford (2008). *FSL 4.1 FMRI Software Library*. URL <http://www.fmrib.ox.ac.uk/fsl/fsl/feeds.html>.
- Analysis Group, FMRI, Oxford (2011). *FSLView v3.1*. URL <http://fsl.fmrib.ox.ac.uk/fsl/fslview/>.
- Athinoula A Martinos Center for Biomedical Imaging (2011). *FreeSurfer v5.1.0*. URL <http://surfer.nmr.mgh.harvard.edu/>.
- Bordier C, Dojat M, Lafaye de Micheaux P (2011). “Temporal and Spatial Independent Component Analysis for fMRI Data Sets Embedded in the **AnalyzeFMRI** R Package.” *44*(9), 1–24. URL <http://www.jstatsoft.org/v44/i09/>.
- Chambers JM (2008). *Software for Data Analysis: Programming in R*. Springer-Verlag, New York.
- Clayden J (2010). *tractor.base: A Package for Reading, Manipulating and Visualising Magnetic Resonance Images*. R package version 1.5.0, URL <http://CRAN.R-project.org/package=tractor.base>.
- Clayden J (2011). *RNiftyReg: Medical Image Registration Using the NiftyReg Library*. R package version 0.3.1, based on original code by Marc Modat and Pankaj Daga, URL <http://CRAN.R-project.org/package=RNiftyReg>.
- Clayden JD, Muñoz Maniega S, Storkey AJ, King MD, Bastin ME, Clark CA (2011). “**TractoR**: Magnetic Resonance Imaging and Tractography with R.” *Journal of Statistical Software*, *44*(8), 1–18. URL <http://www.jstatsoft.org/v44/i08/>.
- Feng D, Tierney L (2011). *mrirc: MRI Tissue Classification*. R package version 0.3-3, URL <http://CRAN.R-project.org/package=mrirc>.
- Ferreira da Silva A (2010a). *cudaBayesreg: CUDA Parallel Implementation of a Bayesian Multilevel Model for fMRI Data Analysis*. R package version 0.3-9, URL <http://CRAN.R-project.org/package=cudaBayesreg>.
- Ferreira da Silva A (2010b). *dpmixsim: Dirichlet Process Mixture Model Simulation for Clustering and Image Segmentation*. R package version 0.0-5, URL <http://CRAN.R-project.org/package=dpmixsim>.

- Ferreira da Silva AR (2011). “**cudaBayesreg**: Parallel Implementation of a Bayesian Multilevel Model for fMRI Data Analysis.” *Journal of Statistical Software*, **44**(4), 1–24. URL <http://www.jstatsoft.org/v44/i04/>.
- Friston KJ, Holmes AP, Poline JB, Grasby PM, Williams SCR, Frackowiak RSJ, Turner R (1995). “Analysis of fMRI Time Series Revisited.” *NeuroImage*, **2**, 45–53.
- Friston KJ, Holmes AP, Worsley KJ, Poline JP, Frith CD, Frackowiak RSJ (1994). “Statistical Parametric Maps in Functional Imaging: A General Linear Approach.” *Human Brain Mapping*, **2**, 189–210.
- Granert O (2010). **Rniftilib**: R Interface to **nifticlib** (V1.1.0). R package version 0.0-29, URL <http://CRAN.R-project.org/package=Rniftilib>.
- Kitware, Inc (2011). **VolView 3.4**. URL <http://www.kitware.com/products/volvview.html>.
- Marchini JL, Lafaye de Micheaux P (2009). **AnalyzeFMRI**: Functions for Analysis of fMRI Datasets Stored in the ANALYZE or NIFTI Format. R package version 1.1-11, URL <http://CRAN.R-project.org/package=AnalyzeFMRI>.
- Nolf E (2003). “**XMedCon** – An Open-Source Medical Image Conversion Toolkit.” *European Journal of Nuclear Medicine*, **30**(Suppl. 2), S246. URL <http://xmedcon.sourceforge.net/>.
- R Development Core Team (2010). *R: A Language and Environment for Statistical Computing*. R Foundation for Statistical Computing, Vienna, Austria. ISBN 3-900051-07-0, URL <http://www.R-project.org/>.
- Rorden C (2011). **MRICro Software Guide**. Version 1.40 build 1, URL <http://www.MRIcro.com/>.
- Sklyar O, Huber W (2006). “Image Analysis for Microscopy Screens.” *R News*, **6**(5), 12–16. URL <http://CRAN.R-project.org/doc/Rnews/>.
- Sklyar O, Pau G, Smith M, Huber W (2010). **EBImage**: Image Processing Toolbox for R. R package version 3.5.5, URL <http://www.Bioconductor.org/packages/release/bioc/html/EBImage.html>.
- Smith J (2011). **MRIConvert**: A Nifty DICOM File Converter. Lewis Center for Neuroimaging, University of Oregon, URL <http://lcni.uoregon.edu/~jolinda/MRIConvert/>.
- Smith SM, Jenkinson M, Woolrich MW, Beckmann CF, Behrens TEJ, Johansen-Berg H, Bannister PR, Luca MD, Drobnjak I, Flitney DE, Niazy R, Saunders J, Vickers J, Zhang Y, Stefano ND, Brady JM, Matthews PM (2004). “Advances in Functional and Structural MR Image Analysis and Implementation as FSL.” *NeuroImage*, **23**(Supplement 1), 208–219.
- Tabelow K, Polzehl J (2011). “Statistical Parametric Maps for Functional MRI Experiments in R: The Package **fmri**.” *Journal of Statistical Software*, **44**(11), 1–21. URL <http://www.jstatsoft.org/v44/i11/>.

Temple Lang D (2010). ***XML**: Tools for Parsing and Generating XML within R and S-PLUS*. R package version 3.1-0, URL <http://CRAN.R-project.org/package=XML>.

Whitcher B, Schmid VJ (2011a). ***dcemriS4**: A Package for Medical Image Analysis*. R package version 0.43, URL <http://CRAN.R-project.org/package=dcemriS4>.

Whitcher B, Schmid VJ (2011b). “Quantitative Analysis of Dynamic Contrast-Enhanced and Diffusion-Weighted Magnetic Resonance Imaging for Oncology in R.” *Journal of Statistical Software*, **44**(5), 1–29. URL <http://www.jstatsoft.org/v44/i05/>.

Whitcher B, Schmid VJ, Thornton A (2011). “Working with the DICOM and NIfTI Data Standards in R.” *Journal of Statistical Software*, **44**(6), 1–28. URL <http://www.jstatsoft.org/v44/i06/>.

Yushkevich PA, Piven J, Cody Hazlett H, Gimpel Smith R, Ho S, Gee JC, Gerig G (2006). “User-Guided 3D Active Contour Segmentation of Anatomical Structures: Significantly Improved Efficiency and Reliability.” *Neuroimage*, **31**(3), 1116–1128.

### Affiliation:

Brandon Whitcher  
Mango Solutions  
Office 202, Second Floor  
14 Greville Street  
London EC1N 8SB, United Kingdom  
E-mail: [bwhitcher@mango-solutions.com](mailto:bwhitcher@mango-solutions.com)  
URL: <http://www2.imperial.ac.uk/~bwhitche/>,  
<http://rigorousanalytics.blogspot.com/>

Volker J. Schmid  
Bioimaging Group  
Department of Statistics  
Ludwig-Maximilians-Universität München  
80539 München, Germany  
E-mail: [volker.schmid@lmu.de](mailto:volker.schmid@lmu.de)  
URL: <http://volkerschmid.de/>

Andrew Thornton  
Cardiff University School of Medicine

Heath Park  
Cardiff CF14 4XN, United Kingdom  
E-mail: [art27@cantab.net](mailto:art27@cantab.net)